

Iron-Selective Electrode Based on Phosphorylated Calix-6-Arene Derivative

Mohsen M. Zareh^{1,2*}, Wael Zordek¹, Ahmed Abd-Alhady¹

¹Department of Chemistry, Faculty of Science, Zagazig University, Zagazig, Egypt

²Department of Chemistry, Faculty of Science, Tabuk University, Tabuk, Saudi Arabia

Email: *mohsenzareh@hotmail.com, *mmzareh@ut.edu.sa, *mmzareh@zu.edu.eg

Received 24 October 2014; revised 24 November 2014; accepted 23 December 2014

Copyright © 2014 by authors and Scientific Research Publishing Inc.

This work is licensed under the Creative Commons Attribution International License (CC BY).

<http://creativecommons.org/licenses/by/4.0/>



Open Access

Abstract

The construction and performance characteristics of a novel Iron(III) membrane sensor based on (37-bis-[(diethoxy-thiophosphoryl)-oxy]-5,11,17,23,29,35-hexakis-(1,1-dimethylethyl)-calix[6]-arene-38,39,40,41,42-pentol) (A) were reported in this paper. The sensor was prepared by incorporating compound (A) into a plasticized polyvinyl chloride PVC membrane. The electrode reveals a Nernstian behavior over a wide iron ion concentration range (1.0×10^{-2} - 1.0×10^{-4} mol·L⁻¹), and relatively low detection limit (1.0×10^{-5} mol·L⁻¹). The potentiometric response was independent on the pH of the solution in the range of 4 - 7. The electrode showed a very short response time (<5 s). It exhibited very good selectivity relative to a wide variety of metal cations. Correlation of selectivity coefficient values with ionic radii of interferent cations was discussed. The proposed iron-ISE was applied for analysis of iron containing samples with comparison to a recommended spectrophotometric method.

Keywords

Ferric Ion Determination, Ion Selective Electrode (ISE), PVC-Membrane

1. Introduction

Different ionophores were used for preparing iron ion-selective electrodes. Benzilthiocarbohydrazide [1] and N-(2-hydroxyethyl) ethylenediamine-N,N',N''-triacetic acid [2] were used as sensor materials for preparing a PVC (polyvinyl chloride) membrane ferric ISE by Zamani *et al.* They only worked up to pH 4.5, although they had very sensitive linear ranges (10^{-2} - 10^{-7} and 10^{-2} - 10^{-9} M). Both electrodes had a life time of more than 10 weeks. Zareh *et al.* [3] used 1-pyrrolidine dicarbothioate for preparing Fe-ISE for the determination of iron in lubrication oil. This electrode showed trivalent Nernstian slope at concentration range 10^{-5} - 10^{-1} M. Benzo-

*Corresponding author.

18-crown-6 was applied as the sensor material for an Iron(III) ion selective electrode by Ekmekci *et al.* [4]. The slope of that electrode was monovalent slope (57 mV/decade). The electrode was responding to FeCl_4^- as an anion electrode. It had a life time up to 2 months. An Iron(III) ion-selective based on a μ -bis-(tridentate) ligand (2-phenyl-1,3-bis [3'-aza-4'-(2'-hydroxyphenyl)-prop-4-en-1'-yl]-1,3-imidazolidine) was constructed by Gupta *et al.* [5]. It had a working pH range 3.5 - 5.5. The age of this electrode was 2 months. Sil *et al.* [6] prepared a coated-wire iron (III) ion-selective electrode based on iron complex of 1,4,8,11-tetraazacyclotetradecane. The slope of that electrode was monovalent (60 ± 5 mV/decade), with a pH working range 1.5 - 3.5. A novel ion selective potentiometric sensor for direct determination of Fe(III) in the presence of Fe(II) was constructed by Mashhadizadeh *et al.* [7]. It was based on 2-[(2-hydroxy-1-propenyl-buta-1,3-dienylimino)-methyl]-4-p-tolylazophenol as a neutral carrier. It showed a super-Nernstian behavior (28.5 mV/decade) for at least 2 months. It works within pH range 4.5 - 6.5. Mahmoud [8] applied iron ion-selective electrodes for direct potentiometry and potentiometric titrimetry in pharmaceuticals. The electrode was based on ion association complexes of Iron(II) 2,4,6-tri (2-pyridyl)-1,3,5-triazine with tetraphenylborate or phosphotungstic acid. In addition, plasticized carboxylated PVC was applied for this membrane. It worked within a pH range 3.2 - 7.1 and a life time of 3 months. Ribonucleic acid as a novel ionophore for potentiometric membrane sensors of some transition metal ions was used by Hassan *et al.* [9]. It showed a Nernstian behavior toward Fe^{2+} (35.5 mV/decade) over a pH range 4.0 - 6.5 (for 10^{-6} - 10^{-2} M). Ferroin-TPB was applied as a membrane sensor for the potentiometric determination of either Fe^{2+} or Fe^{3+} ion by Hassan and Marzouk [10]. This type of sensor was based on responding to the charged ion complex "ferrion". It behaved like a cationic divalent electrode (30 mV/decade). It showed a pH range 3 - 9 down to 4×10^{-7} M ferrion.

The present iron electrodes were constructed depending on the use of (37-bis-[(diethoxy-thiophosphoryl)oxy]-5,11,17,23,29,35-hexakis-(1,1-dimethylethyl)-calix[6]arene-38,39,40,41,42-pentol) (A), "Figure 1". Here, the study is elaborated for studying the effect of ionic radii of interferent cations to their selectivity coefficient values towards ferric ion. The application of this electrode facilitates the measurement and analysis of ferric ion in different samples. None of the previous work suggested the use of calix-6-arene for iron determination.

2. Experimental

2.1. Reagents and Material

37-bis-[(diethoxy-thiophosphoryl)oxy]-5,11,17,23,29,35-hexakis(1,1-dimethyl-ethyl)-calix[6]arene-38,39,40,41,42-pentol (A) synthesized according to a previous procedure (kindly provided by Prof. Z. Bozoka, Warsaw Technical Univ., Poland) [11], and tetra-p-chlorophenylborate (B) [Fluka] were the main ionophores for preparing the applied membranes. The used plasticizers were dioctylsebacate (DOS) [Aldrich], nitrophenyloctylether (NPOE) [Fluka]. Polyvinylchloride (PVC) [Fluka] was the membrane matrix. The membrane components were dissolved in tetrahydrofuran (THF) [Fluka]. A (0.1 M) standard stock solutions of ferric chloride [Aldrich] was prepared and dilutions were made to cover the required range (10^{-2} - 10^{-7} M). To perform the selectivity studies, the analytical reagent grade of nitrates of Na^+ , K^+ , NH_4^+ , Ag^+ , Ni^{2+} , Hg^{2+} , Cu^{2+} , Zn^{2+} , Co^{2+} , Cd^{2+} , Pb^{2+} , Sr^{2+} , Mg^{2+} , Ca^{2+} and Al^{3+} were used. Diluted solutions (10^{-2} - 10^{-4} M) were obtained by careful dilution of the standard

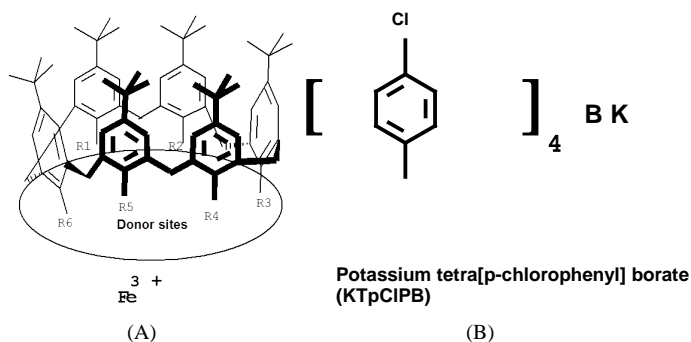


Figure 1. Structural formulas of: (A) 37-bis-[(diethoxy-thiophosphoryl)oxy]-5,11,17,23,29,35-hexakis-(1,1-dimethylethyl)-calix[6]arene-38,39,40,41,42-pentol; (B) potassium tetrakis-[3,5-bis-(trifluoro-methyl)-phenyl] borate.

stock solution. Double distilled water was used throughout.

2.2. Equipment


The potentiometric/pH-measurements were carried out (at $25^{\circ}\text{C} \pm 1^{\circ}\text{C}$) on a digital research pH-meter (Jenway, UK) (sensitivity, ± 0.1 mV) coupled with a channel selector. The spectrophotometric measurements were carried using (UV1800-Schimidzu-Japan).

2.3. Electrode Preparation

The measurement was carried using an electrode, which was assembled using Teflon tube (length = 10 cm, diameter = 4 mm) fitted with PVC-tube end. Three membrane compositions (I-III) were tried 1% w/w ionophore (either A or B); 33% w/w PVC and 66% w/w solvent mediators (NPOE) or (DOS). These components were dissolved in THF and poured into glass rings of 4 cm i.d. resting on a glass plate. The mixture was left overnight for evaporation, and then the resulting membrane was cut into discs of 6 mm i.d. Each disc was fixed to the end of PVC-tube at the end of the electrode. The electrode-compartment was filled with an aqueous inner filling solution (0.01 M ferric nitrate and KCl) IF. “Table 1”, showed the composition of membranes used for preparing the iron—ISE. For electrode conditioning, it was soaked for 24 h into 1×10^{-2} M solution of Fe^{3+} before use.

2.4. Potentiometric Measurements

25 ml aliquots of Fe^{3+} solution (10^{-7} - 10^{-1} M) were transferred to 50 ml beakers in presence of 0.1 M KNO_3 for ionic strength adjustment and buffered at pH5 using acetate-buffer solution. The ferric-ISE was dipped into the solution in conjunction with Ag-AgCl double junction reference electrode (Orion model 900200). The cell potential was recorded corresponding to each Fe^{3+} -concentration. A calibration graph can be constructed for the cell potential versus $-\log(\text{Fe}^{3+})$. The following cell assembly was applied:



The potentiometric selectivity coefficient ($K_{\text{Fe}^{3+}, \text{X}^{Z+}}^{\text{Pot}}$) values for different common cations were determined by the separate solution method [12] (10^{-3} M solutions for both iron and interferent). The pH-effect on the potential of the proposed electrode was studied by recording the potential after adjusting the pH of tested solutions using 0.1 M KOH or 0.1 M HCl.

2.5. Determination of Iron in Its Samples Using ISE- Fe^{3+}

Different iron-containing samples were prepared. The standard addition method was used for analysing these samples by using the proposed electrode. The samples were previously treated with HCl to referee the complexed iron. The method based on addition of known standard (0.558 ppm) to the unknown samples. Then the mV-measurements were conducted by the proposed iron selective electrode. The obtained readings were compared to previously prepared calibration graph covering the measured concentration range (0.5618 - 0.926 ppm).

For evaluation of the proposed electrode and the accuracy, results from another recommended method was conducted. The samples were analysed by spectrophotometric method [13] for comparison. The procedure was based on addition of 2 ml HCl and add 1 ml $\text{NH}_2\text{OH-HCl}$ to 50 ml of sample. Boil the sample until it becomes 15 - 20 ml then cool. Transfer the solution to a volumetric flask. Add 10 ml amm. acetate and 4 ml 1,10-phenanthroline to the exit solution and complete to 50 ml with distilled water. Wait 10 min. until the color appears. Then, the samples were measured by using spectrophotometer.

Table 1. Composition of membranes I, II and III used for preparing ion selective electrode for Iron(III).

Composition, w/w%	PVC	DTPCX	TpCIPB	DOS	NPOE	% ionophore	Slope, mV/decade
I-membrane	60	1	1.2	0	120	1.206	48
II-membrane	60	1.4	1.6	121	0	1.630	32
III-membrane	61.2	2.7	0	0	121.8	1.475	22

3. Results and Discussion

3.1. Effect of Composition

Different membrane compositions were prepared for optimization of the best one. Electrodes I and II comprised the membrane with NPOE plasticizer, while electrode-III comprised membrane with DOS as plasticizer. Compound (B) was a charged additive for the sensor material of electrodes I and II, while (B) was the only main ionophore for III.


By comparing the electrodes I and II, after 1 day soaking, the slope of type I was 59 mV/decade, while for type II it was 15 mV/decade. This is because both electrodes had different plasticizers (NPOE and DOS), which played an important role in the electrode response [14]. “Figure 2” shows calibration graphs for the three membrane types. It can be reported that NPOE had an active exchange site that works as an ionophoric group. For electrode type I both B and NPOE played a role in the electrode behavior. Double effect resulted in the high value of the slope 59 mV/decade, but when only TpCIB was present the slope decreased 50% reaching 30 mV/decade.

After 6 days, the slope values for electrodes (types I and III) with NPOE decreased, while it increased for electrode II. The decrease in slope values for I and II is due to usual leaching out of membrane components. For membrane II, the increase in slope can be attributed to the slow interaction between Fe^{3+} and membrane ionophore as a result of the presence of DOS.


After prolonged soaking (2 months) electrode I lost the monovalent response, electrode II lost the divalent response, while electrode III reserved its trivalent response.

The detection limit (DL) of an ISE can be defined as the cross point of lines segments fitted to linear segments of emf vs $\log a_{\text{Fe}^{3+}}$ [12]. For membrane-III, the recorded DL was 1.2×10^{-5} M after 1 day soaking time. It reached 3.9×10^{-6} M after 2 months. The DL reached 6.3×10^{-7} for electrode I after 42 days continuous soaking. “Table 2”, shows the obtained results.

Mechanism of the electrode response comprises only A-ionophore can be represented as:

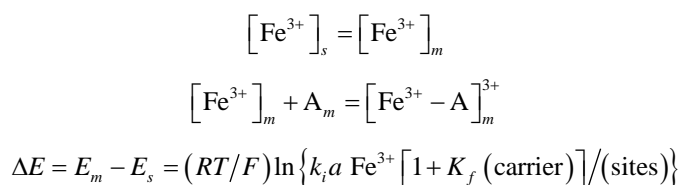

where: m refers to the membrane site, and s refers to the solution site. When the membrane comprises both A and B the mechanism follow the scheme below:

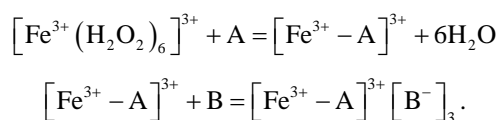

Response time was estimated according to IUPAC definition [12]. It is the time between the instant when the electrode was brought into contact with sample solution and the first instant when emf/time slope becomes equal to the limiting value selected on the basis of experimental conditions. Dynamic response of the proposed electrode is shown in “Figure 3”. From the figure it is shown that response time is between 5 - 10 s for the measured concentrations between 10^{-2} - 10^{-4} M.

3.2. pH-Effect

The potential changes versus different pH-values for the three kinds of the membranes were studied. It can be detected that the acidic part differs for type III electrode than others (types I and II). The break at this part occurs at pH values 3.6, 3.9 and 4.5 to 7 for I, II and III electrodes, respectively. The sensitivity of penta-thiophosphorylatedcalix[6]arene (A) towards the H^+ is the reason for the absence of the plateau potential in acidic medium for type III membrane electrode. The break in acidic medium is due to the protonation of the corresponding ionophore in the membrane. Under these conditions the iron complex cannot be formed. Representative curves are shown for the proposed iron-ISE with membrane types II and III are shown in “Figure 4” and “Figure 5”.

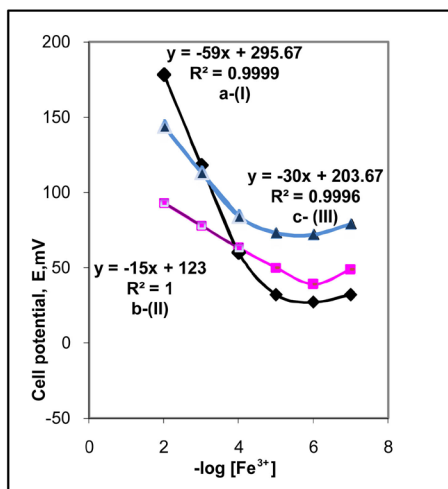


Figure 2. Calibration graphs for iron-ISE comprising: (a) Membrane-I; (b) Membrane-II; (c) Membrane-III.

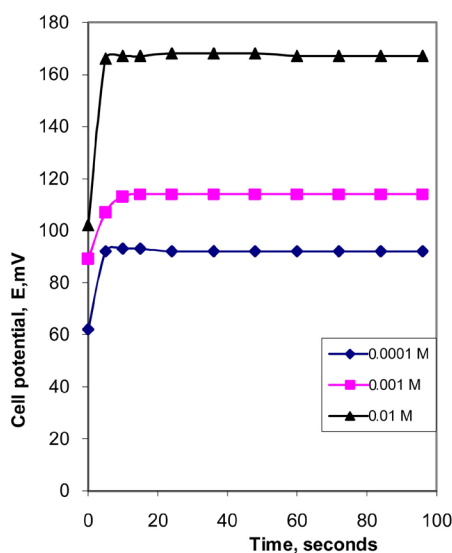


Figure 3. Dynamic response of iron-ISE with membrane type III when measuring Fe^{3+} solutions with concentrations 0.01, 0.001, and 0.0001 M.

Table 2. Effect of soaking on ferric-ISE-response based on TpCIPB ionophore comprising either DOS/or NPOE.

Soaking time	I				II				III			
	Slope	R ^{2b}	LR ^a , M	DL, M	Slope	R ^{2b}	LR ^a , M	DL, M	Slope	R ^{2b}	LR ^a , M	DL, M
1 day	59	0.999	10 ⁻² - 2.5 × 10 ⁻⁵	2.0 × 10 ⁻⁵	15	1	10 ⁻² - 1.5 × 10 ⁻⁵	3.1 × 10 ⁻⁷	30	0.999	10 ⁻² - 2.5 × 10 ⁻⁵	1.2 × 10 ⁻⁵
6 days	48	1	10 ⁻² - 2.5 × 10 ⁻⁵	1.5 × 10 ⁻⁵	32	1	10 ⁻² - 1.5 × 10 ⁻⁵	6.3 × 10 ⁻⁶	22	0.993	10 ⁻² - 3.9 × 10 ⁻⁵	1.2 × 10 ⁻⁵
8 days	38.5	0.948	10 ⁻² - 2.5 × 10 ⁻⁶	10 ⁻⁶	39	0.999	10 ⁻² - 2.5 × 10 ⁻⁵	1 × 10 ⁻⁵	24	1	10 ⁻² - 2.5 × 10 ⁻⁵	5.0 × 10 ⁻⁶
42 days	36.5	0.9895	10 ⁻² - 1.5 × 10 ⁻⁶	6.3 × 10 ⁻⁷	32	0.9987	10 ⁻² - 1.0 × 10 ⁻⁵	2.5 × 10 ⁻⁶	25	0.9586	10 ⁻² - 2.5 × 10 ⁻⁵	5.0 × 10 ⁻⁶
2 months	39	0.992	10 ⁻² - 1 × 10 ⁻⁵	3.9 × 10 ⁻⁶	47	0.999	10 ⁻² - 6.3 × 10 ⁻⁵	1.5 × 10 ⁻⁵	25.5	0.999	10 ⁻² - 3.9 × 10 ⁻⁵	3.9 × 10 ⁻⁶

^aLinear range. ^bCorrelation coefficient.

It is observed that the plateau potential is more flat for the electrode with membrane type II than in membrane type III. This is expected due to the absence of (B) in the membrane type III.

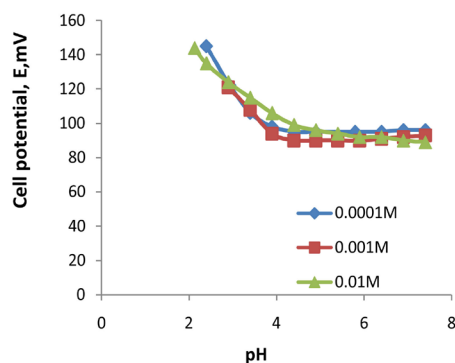


Figure 4. pH-effect on potential of iron-ISE with membrane type II when measuring Fe^{3+} solutions with concentrations 0.01, 0.001, and 0.0001 M.

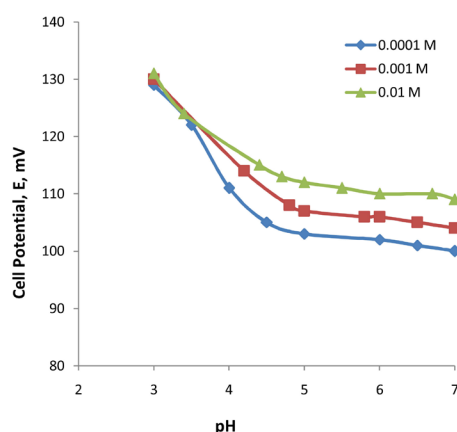


Figure 5. pH-effect on potential of iron-ISE with membrane type III when measuring Fe^{3+} solutions with concentrations 0.01, 0.001, and 0.0001 M.

3.3. Selectivity Properties

The selectivity of Fe-ISE with different membrane types I, II and III were calculated according to the SSM [12]. “Table 3” shows the obtained $K_{\text{Fe}^{3+}, \text{XZ}^+}^{\text{Pot}}$ -values of the selectivity coefficient. It can be reported that most of the tested interferents for Fe-ISE type I shows suitable selectivity. The values of the selectivity coefficients for the ISE-Fe type I towards the tested divalent cations were between $(1.03 \times 10^{-2} - 5.93 \times 10^{-4})$. For Hg^{2+} , good $K_{\text{Fe}^{3+}, \text{XZ}^+}^{\text{Pot}}$ value was found (5.9×10^{-4}) . Monovalent cations showed $K_{\text{Fe}^{3+}, \text{XZ}^+}^{\text{Pot}}$ -values in the range of $(1.1 \times 10^{-1} - 3.1 \times 10^{-1})$, which are relatively higher than the tested divalent cations.

In case of Fe-ISE type II, most of the tested cations showed $K_{\text{Fe}^{3+}, \text{XZ}^+}^{\text{Pot}}$ -values of the order of $\approx 10^{-3}$. This means that the electrode can be applied for measurements in their presence. Monovalent cations like NH_4^+ exhibits $K_{\text{Fe}^{3+}, \text{XZ}^+}^{\text{Pot}}$ -value of order of 10^{-2} , while Na^+ and Ag^+ showed $K_{\text{Fe}^{3+}, \text{XZ}^+}^{\text{Pot}}$ -value of order 10^{-1} .

It can be concluded that the type of plasticizer affects the selectivity properties of the electrodes.

When Fe-ISE type III that contains only A/NPOE without B, improvements of $K_{\text{Fe}^{3+}, \text{XZ}^+}^{\text{Pot}}$ -values were observed for the most divalents and monovalent cations, except for Ag^+ , compared to other electrodes (I and II).

The relation between ionic radius of interferent cations and the values of selectivity coefficient is shown in “Figure 6”. It is found that the relation has a maximum $K_{\text{Fe}^{3+}, \text{XZ}^+}^{\text{Pot}}$ -value (0.237) at ionic radius 129 pm (for Ag^+) for the electrode type III in the three concentrations (0.01, 0.001, and 0.0001M) [15]. Less values were ob-

served either when ionic radius is less or more than 129 pm. This can be explained due to that Ag^+ fits the ionophore cavity, which results in highest interaction. The same behavior was proved for the Fe-ISE with membrane types I and II. The highest $K_{\text{Fe}^{3+}, \text{X}^{Z+}}^{\text{Pot}}$ -value was observed for Ag^+ . “Figure 7” shows the variations of $K_{\text{Fe}^{3+}, \text{X}^{Z+}}^{\text{Pot}}$ -values according to the ionic radius of the tested cations at different concentrations.

3.4. Application of Fe-ISE for Determining Iron in Actual-Like Samples

Ten iron-containing samples were analysed for iron by using the proposed electrode “Fe-ISE”. The procedure was based on the standard addition method. Most of the obtained results were between 0.02 and 0.078 ppm. Only samples 8 and 9 were much higher (0.12 and 0.37 ppm). The obtained results agreed with those obtained from a spectrophotometric method based on 1,10-phenanthroline according to previously discussed procedures [13]. “Table 4”, shows the obtained results for analysis by using both the proposed electrode and the spectrophotometric methods.

Table 3. Selectivity coefficient values for iron electrodes based on (A + B/NPOE) [I], (A + B/DOS) [II], (A/NPOE) [III] membranes, when measuring 0.001 M ferric/interferent solution.

Interferent	Ionic radius	$K_{\text{Fe}^{3+}, \text{X}^{Z+}}^{\text{Pot}}$		
		I	II	III
Ca^{2+}	114	0.003162	0.004084	0.001468
Cd^{2+}	109	0.00194	0.005995	0.001468
Ba^{2+}	149	0.016518	0.008424	0.004338
Sr^{2+}	132	0.018588	0.010248	0.004338
Cu^{2+}	87	0.006571	0.005012	0.002746
Mg^{2+}	86	0.011925	0.009602	0.003314
Hg^{2+}	116	0.000593	0.002154	0.000353
Co^{2+}	87	0.0103	0.008389	0.005926
Mn^{2+}	97 - 81	0.010926	0.008389	0.003899
Pb^{2+}	133	0.001191	0.001896	0.000947
NH_4^+	175	0.182085	0.065097	0.110069
Na^+	116	0.096895	0.112421	0.068129
Ag^+	129	0.012276	0.310117	0.195734

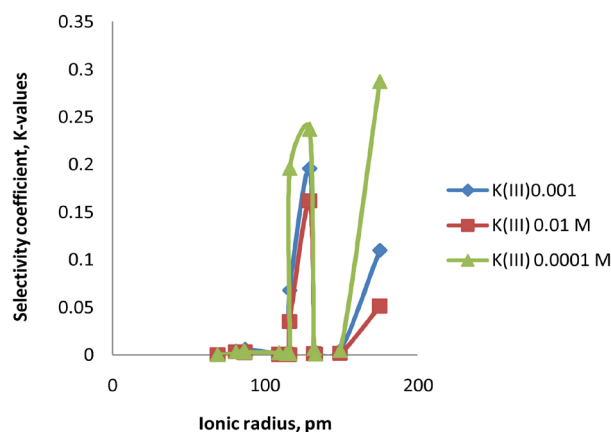


Figure 6. Correlation between ionic radius (pm) of the tested cations and selectivity coefficient ($K_{\text{Fe}^{3+}, \text{X}^{Z+}}^{\text{Pot}}$) for iron-ISE containing membrane type III for iron solutions with concentrations 0.01, 0.001, and 0.0001 M.

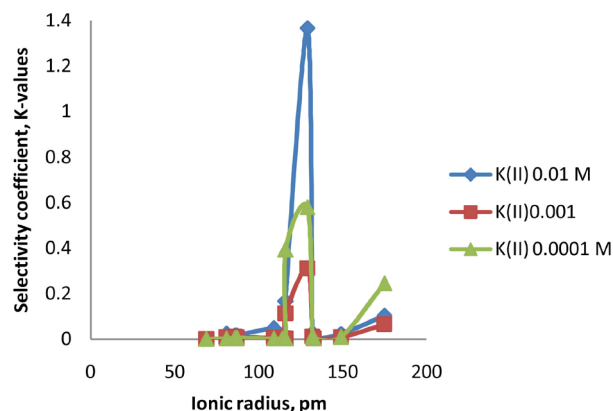


Figure 7. Correlation between ionic radius (pm) of the tested cations and selectivity coefficient ($K_{Fe^{3+}, X^{z+}}^{Pot}$) for iron-ISE containing membrane type II for iron solutions with concentrations 0.01, 0.001, and 0.0001 M.

Table 4. Application of iron-ISE for determination of iron in different samples.

No.	Sample	Fe ³⁺ , ppm		RTD ^a , %
		Spectrophotometric method	Proposed ISE method	
1	Sample (1)	0.050	0.049	2.1
2	Sample (2)	0.060	0.065	1.9
3	Sample (3)	0.022	0.019	1.7
4	Sample (4)	0.022	0.020	1.67
5	Sample (5)	0.081	0.078	1.8
6	Sample (6)	0.0058	0.0057	2.2
7	Sample (7)	0.058	0.052	2.13
8	Sample (8)	0.120	0.120	0.95
9	Sample (9)	0.360	0.370	1.1
10	Sample (10)	0.027	0.025	1.5

^aRelative standard deviation (4-determinations).

4. Conclusion

It can be concluded that iron can be determined by using new sensor based on using new phosphorylated calix-6-arene ionophore. The studies of relation between selectivity and ionic radius of interferences recommend that there is a limit for the ionic radius where the selectivity coefficient values reaches maximum. The electrode was applied successfully for analyzing iron in range of (1×10^{-2} - 1×10^{-4} M). The obtained results agreed with those of a recommended spectrophotometric method [13].

Acknowledgements

The authors acknowledge Prof. Z. Brzozka, Warsaw Technical Univ, Poland, for providing us with phosphorylated calix-6-derivative.

References

- [1] Zamani, H.A., Anjali, G.M.R., Behmadi, H. and Behnajady, M.A. (2009) Fabrication of an Iron(III) PVC-Membrane Sensor Based on Bis-Benzilthiocarbohydrazide as a Selective Sensing Material. *Materials Science and Engineering: C*, **29**, 1535. <http://dx.doi.org/10.1016/j.msec.2008.12.004>
- [2] Zamani, H.A., Hamed-Mosavian, M.T., Hamidfar, E., Ganjali M.R. and Norouzi, P. (2008) A Novel Iron(III)-PVC Membrane Potentiometric Sensor Based on N-(2-Hydroxyethyl)Ethylendiamine-N,N',N''-Triacetic Acid. *Materials Science and Engineering: C*, **28**, 1551. <http://dx.doi.org/10.1016/j.msec.2008.04.013>

- [3] Zareh, M.M., Ismail, F.A.I. and Abd Alaziz, M.H. (2010) 1-Pyrrolidine Dicarbodithioate Based Electrodes for Determination of Iron(III) in Lubrication Oil. *Electroanalysis*, **22**, 1369. <http://dx.doi.org/10.1002/elan.200900550>
- [4] Ekmekci, G., Uzun, D., Somer, G. and Kalaycı, Ş. (2007) A Novel Iron(III) Selective Membrane Electrode Based on Benzo-18-Crown-6 Crown Ether and Its Applications. *Journal of Membrane Science*, **288**, 36. <http://dx.doi.org/10.1016/j.memsci.2006.10.044>
- [5] Gupta, V.K., Jain, A.K., Agarwal, S. and Maheshwari, G. (2007) An Iron(III) Ion-Selective Sensor Based on a μ -bis(Tridentate) Ligand. *Talanta*, **71**, 1964. <http://dx.doi.org/10.1016/j.talanta.2006.08.038>
- [6] Sil, A., Ijeri, V.S. and Srivastava, A.K. (2005) Coated-Wire Iron(III) Ion-Selective Electrode Based on Iron Complex of 1,4,8,11-Tetraazacyclotetradecane. *Sensors and Actuators B: Chemical*, **106**, 648. <http://dx.doi.org/10.1016/j.snb.2004.09.013>
- [7] Mashhadizadeh, M.H., Shoaie, I.S. and Monadi, N. (2004) A Novel Ion Selective Membrane Potentiometric Sensor for Direct Determination of Fe(III) in the Presence of Fe(II). *Talanta*, **64**, 1048. <http://dx.doi.org/10.1016/j.talanta.2004.05.005>
- [8] Mahmoud, W.H. (2001) Iron Ion-Selective Electrodes for Direct Potentiometry and Potentiometric Titrimetry in Pharmaceuticals. *Analytica Chimica Acta*, **436**, 199. [http://dx.doi.org/10.1016/S0003-2670\(01\)00892-3](http://dx.doi.org/10.1016/S0003-2670(01)00892-3)
- [9] Hassan, S.S., Mahmoud, W.H. and Othman, A.H. (1998) Ribonucleic Acid as a Novel Ionophore for Potentiometric Membrane Sensors of Some Transition Metal Ions. *Talanta*, **47**, 377. [http://dx.doi.org/10.1016/S0039-9140\(98\)00142-8](http://dx.doi.org/10.1016/S0039-9140(98)00142-8)
- [10] Hassan, S.S.M. and Marzouk, S.A.M. (1994) A Novel Ferrous Membrane Sensor for Potentiometric Determination of Iron. *Talanta*, **41**, 891. [http://dx.doi.org/10.1016/0039-9140\(94\)E0042-P](http://dx.doi.org/10.1016/0039-9140(94)E0042-P)
- [11] Wroblewski, W. and Brzozka, Z. (1996) Lead versus Cadmium Selectivity of Ion Selective Electrodes Based on Thiophosphorylated Calix[6]Arene Ionophores. *New Journal of Chemistry*, **20**, 419.
- [12] Buck, R.P. and Lindner, E. (1994) Recommendations for Nomenclature of Ionselective Electrodes (IUPAC Recommendations 1994). *Pure and Applied Chemistry*, **66**, 2527. <http://dx.doi.org/10.1351/pac199466122527>
- [13] Eaton, A.D., Clescri, L.S. and Greenberg, A.E. (1995) Standard Methods for Examination of Water and Waste Water. American Public Health Association, Washington DC.
- [14] Zareh, M.M. (2009) Blank Membranes versus Ionophore-Based Membranes for the Selective Determination of H^+ . *Analytical Sciences*, **25**, 1131. <http://dx.doi.org/10.2116/analsci.25.1131>
- [15] Shannon, R.D. (1976) Revised Effective Ionic Radii and Systematic Studies of Interatomic Distances in Halides and Chalcogenides. *Acta Crystallographica*, **A32**, 751. <http://dx.doi.org/10.1107/S0567739476001551>